




# REPLACEMENT SHEET

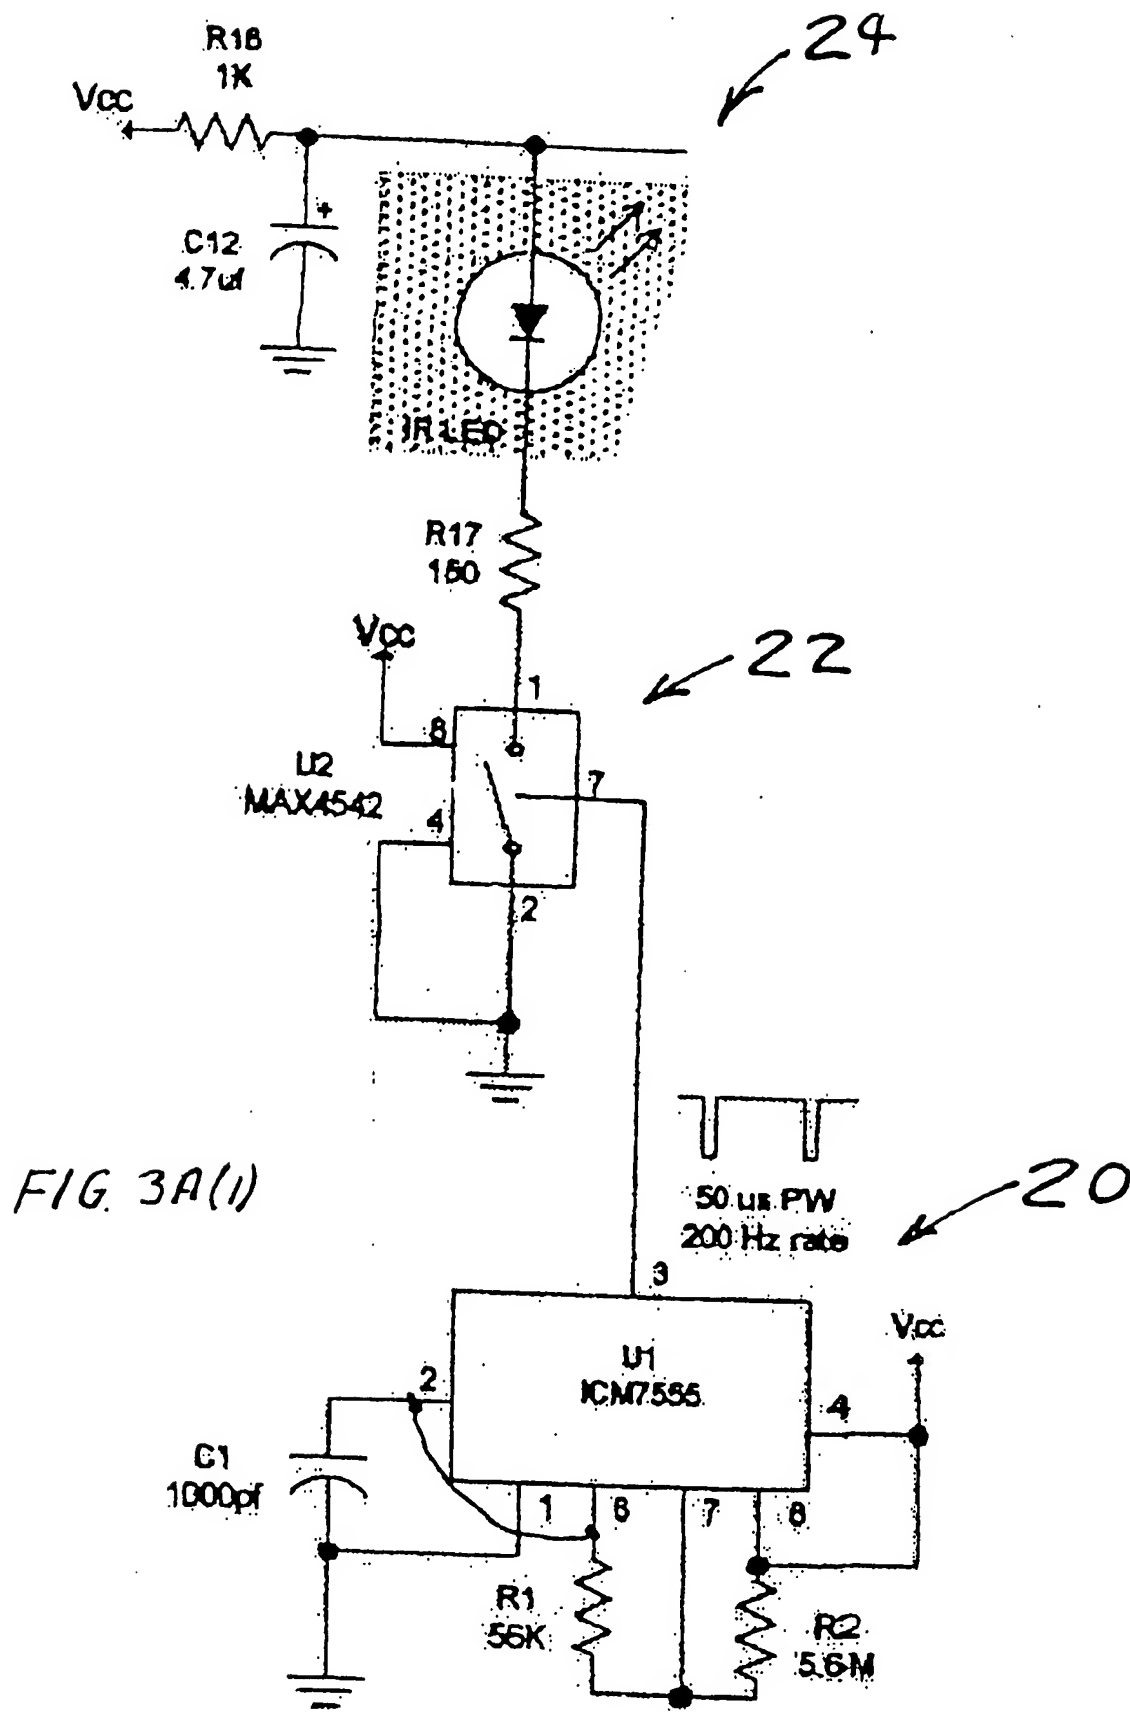


# REPLACEMENT SHEET


FIG. 3A(2)

REFLECTIVE SENSOR

EE-SY-124

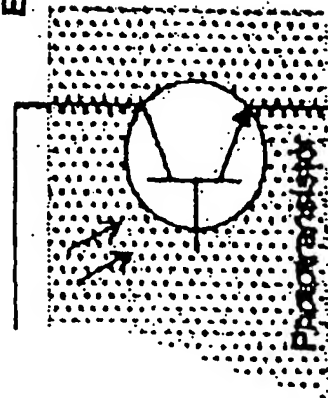


26

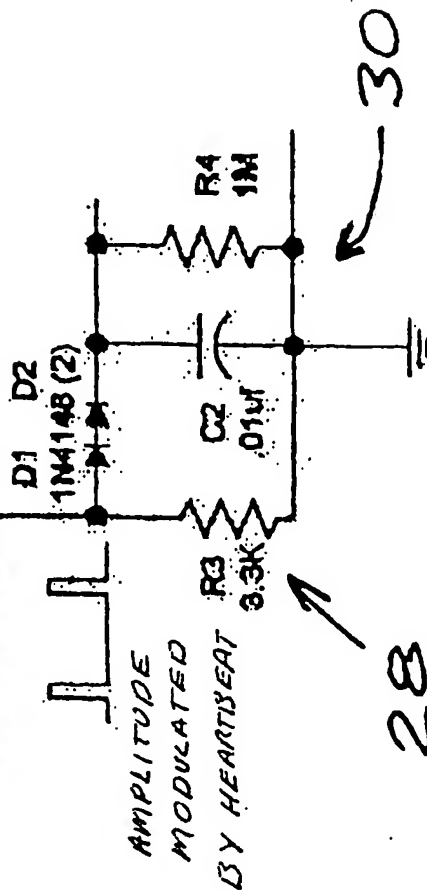

28

FIG. 3A(3)

V<sub>CC</sub>

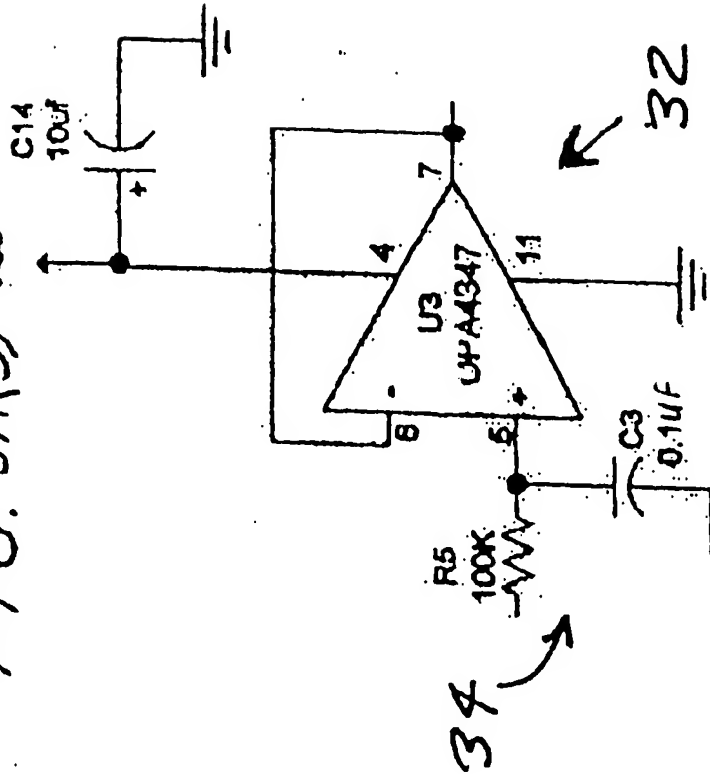


32

34

REPLACEMENT SHEET

FIG. 3A(4)

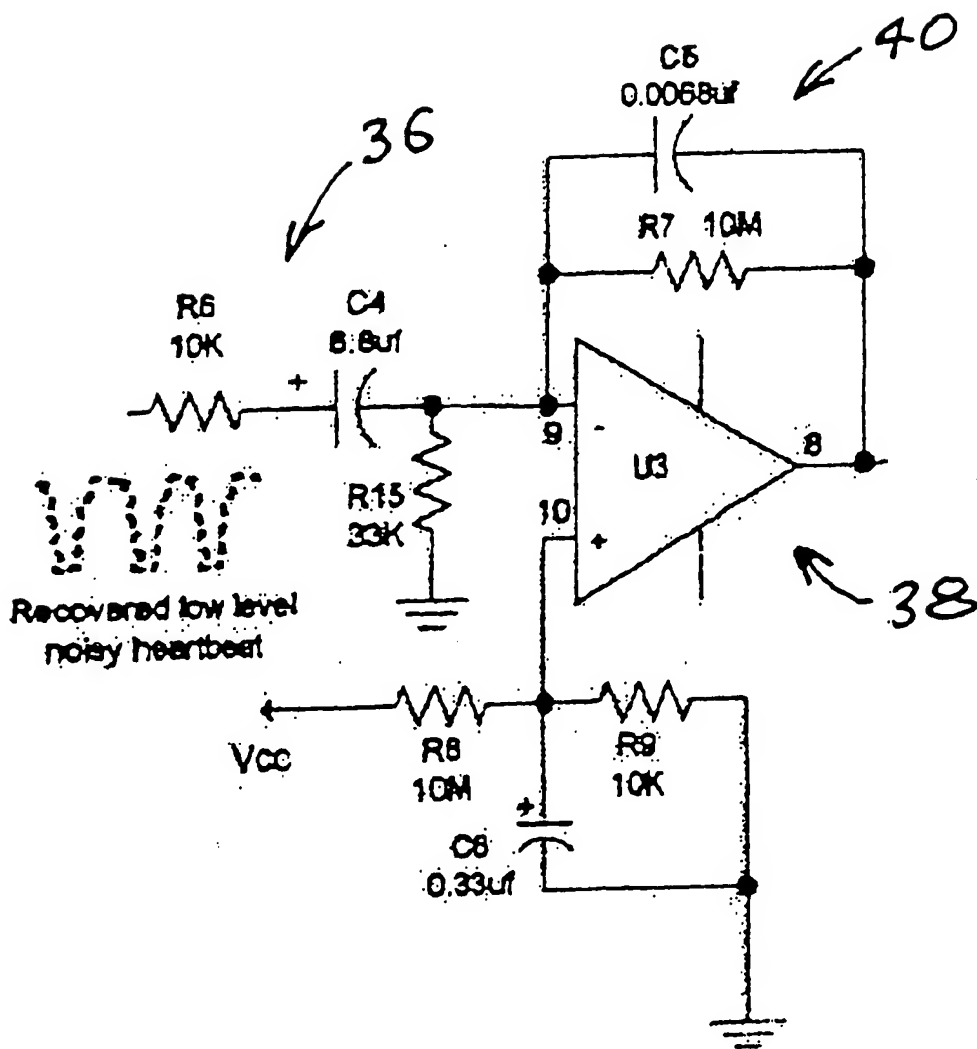

# REPLACEMENT SHEET

FIG. 3A(5)

Amplified and  
Filtered heartbeat



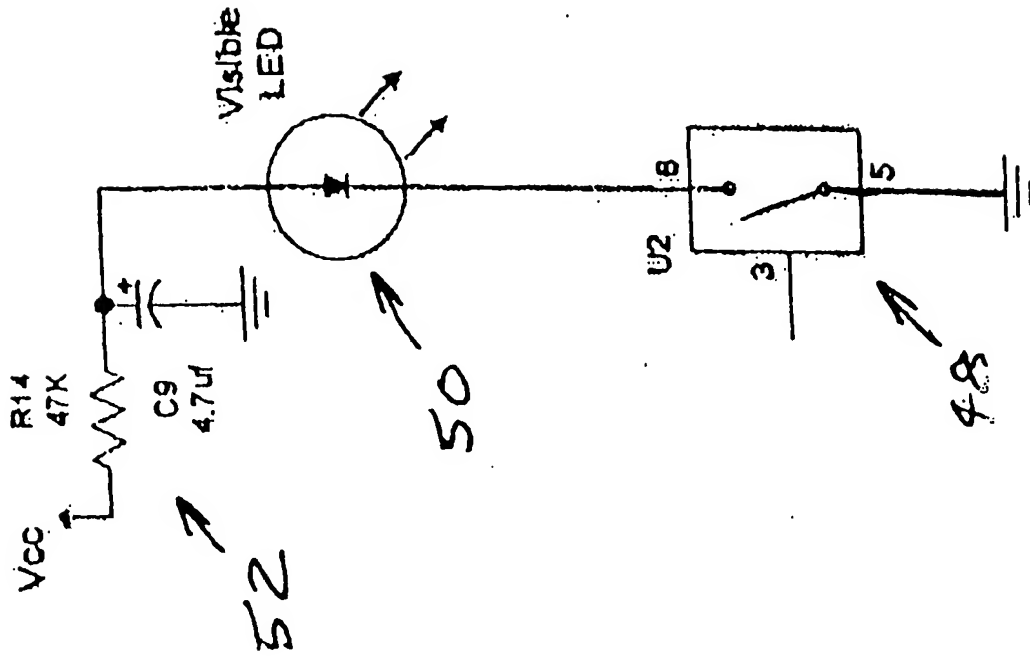


FIG. 3A(6)

# REPLACEMENT SHEET

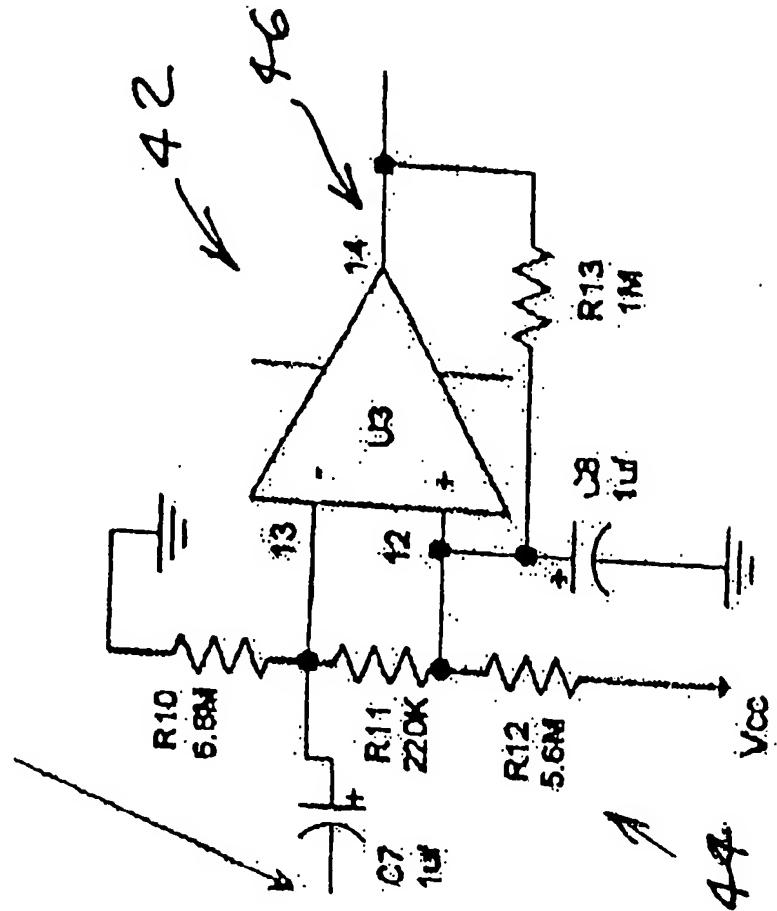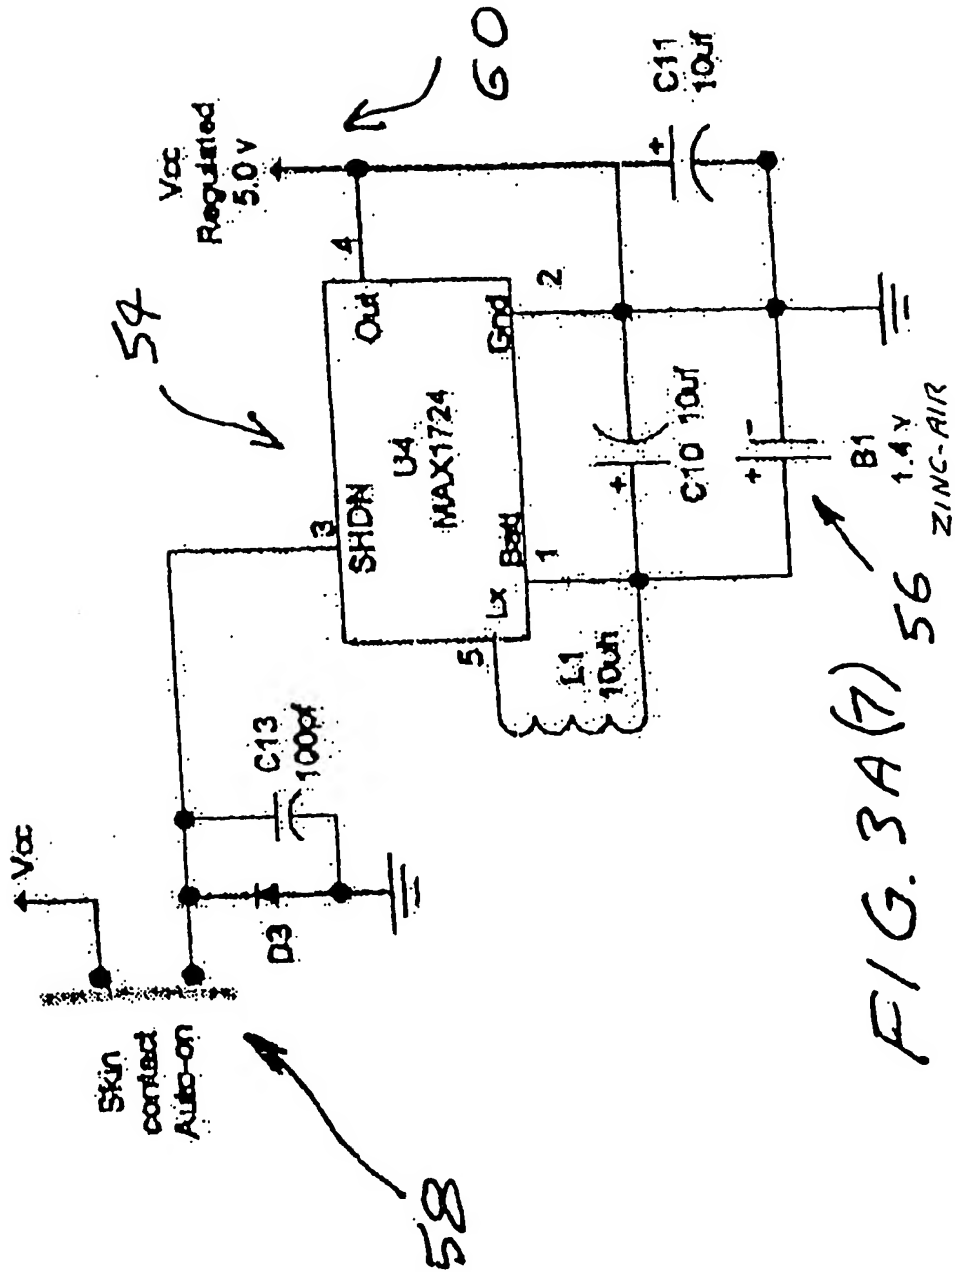

# REPLACEMENT SHEET

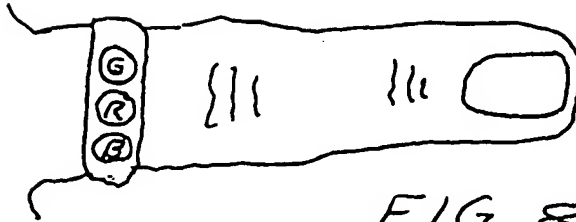


FIG. 8

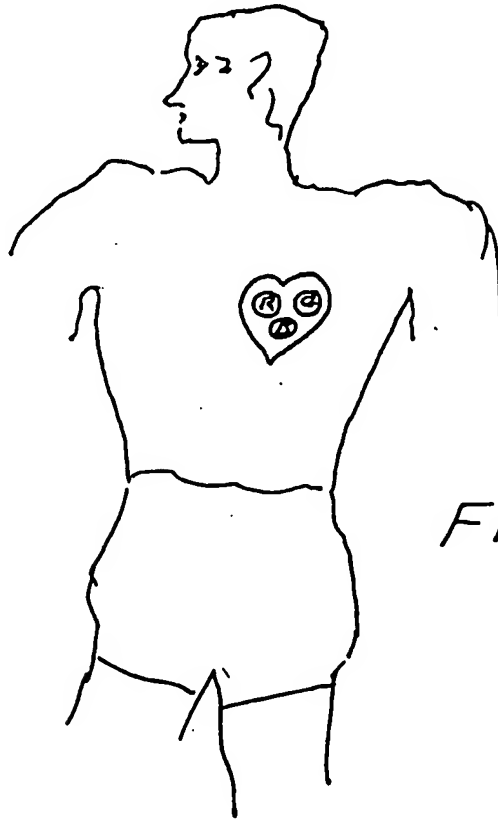


FIG. 9